
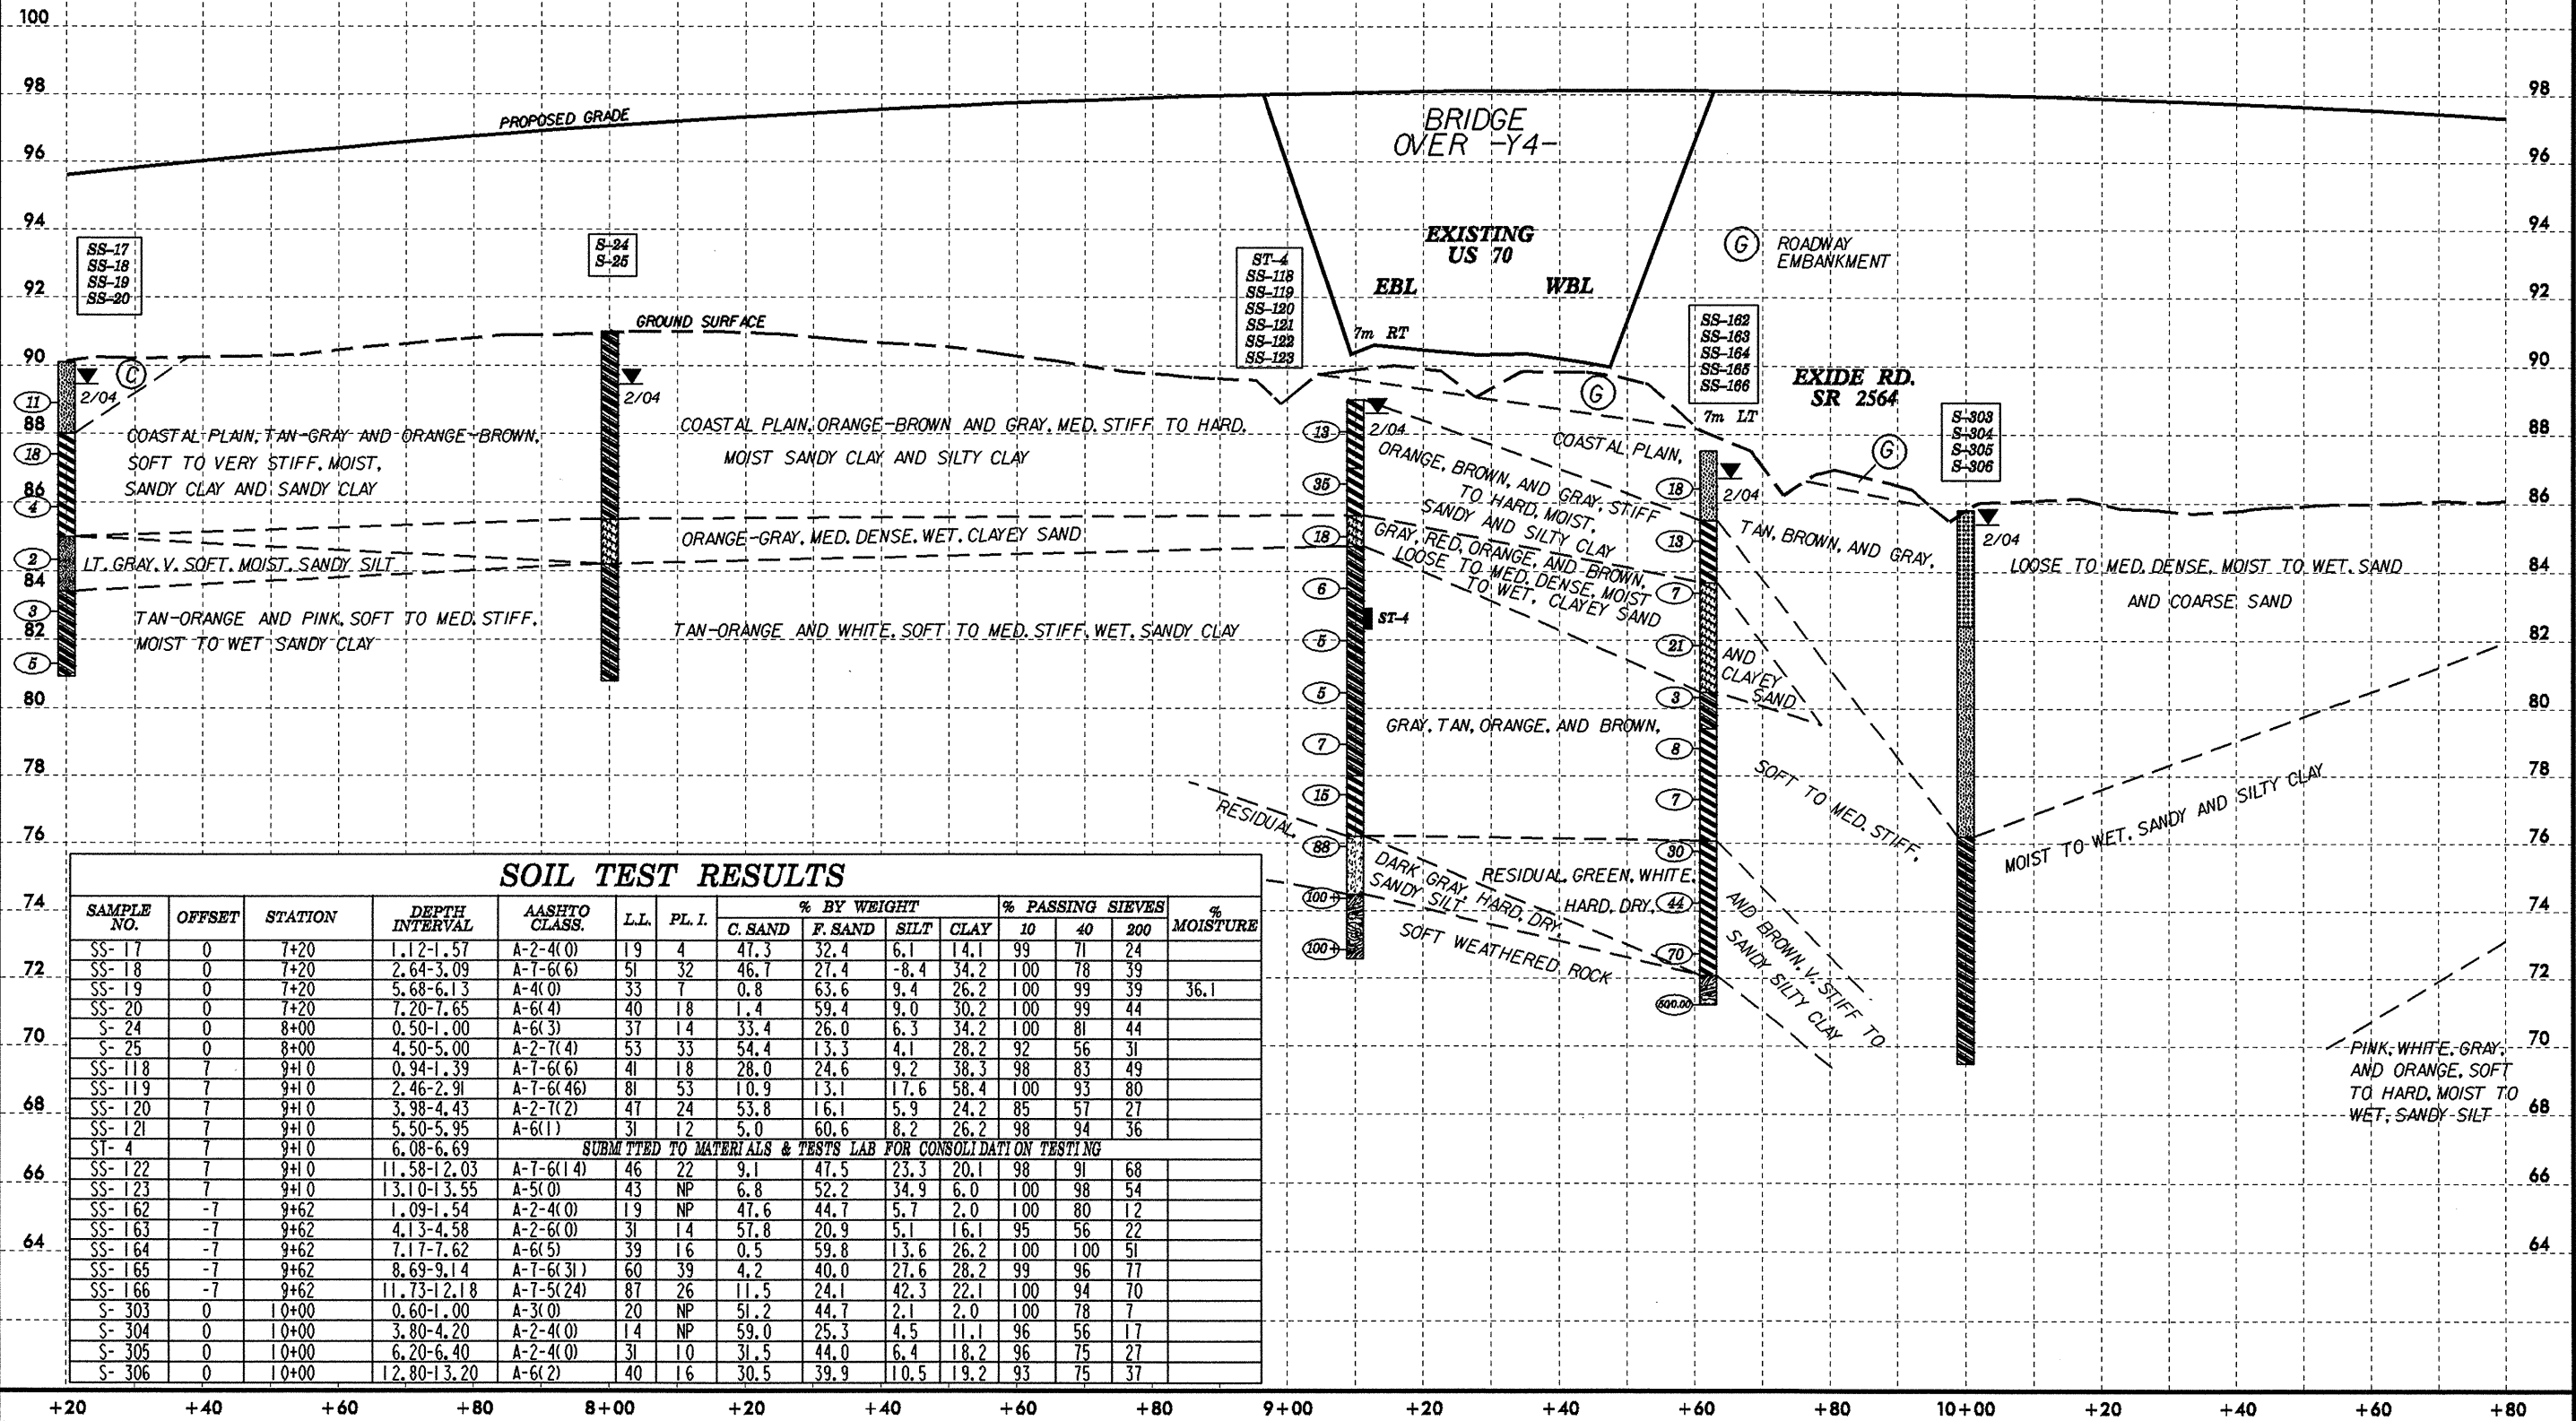


-FLYOVER-



SOIL TEST RESULTS

SAMPLE NO.	OFFSET	STATION	DEPTH INTERVAL	AASHTO CLASS.	L.L.	P.L. I.	% BY WEIGHT				% PASSING SIEVES			% MOISTURE
							C. SAND	F. SAND	SILT	CLAY	10	40	200	
SS-17	0	7+20	1.12-1.57	A-2-4(0)	19	4	47.3	32.4	6.1	14.1	99	71	24	
SS-18	0	7+20	2.64-3.09	A-7-6(6)	51	32	46.7	27.4	-8.4	34.2	100	78	39	
SS-19	0	7+20	5.68-6.13	A-4(0)	33	7	0.8	63.6	9.4	26.2	100	99	39	36.1
SS-20	0	7+20	7.20-7.65	A-6(4)	40	18	1.4	59.4	9.0	30.2	100	99	44	
S-24	0	8+00	0.50-1.00	A-6(3)	37	14	33.4	26.0	6.3	34.2	100	81	44	
S-25	0	8+00	4.50-5.00	A-2-7(4)	53	33	54.4	13.3	4.1	28.2	92	56	31	
SS-118	7	9+10	0.94-1.39	A-7-6(6)	41	18	28.0	24.6	9.2	38.3	98	83	49	
SS-119	7	9+10	2.46-2.91	A-7-6(46)	81	53	10.9	13.1	17.6	58.4	100	93	80	
SS-120	7	9+10	3.98-4.43	A-2-7(2)	47	24	53.8	16.1	5.9	24.2	85	57	27	
SS-121	7	9+10	5.50-5.95	A-6(1)	31	12	60.6	8.2	26.2	98	94	36		
ST-4	7	9+10	6.08-6.69	SUBMITTED TO MATERIALS & TESTS LAB FOR CONSOLIDATION TESTING										
SS-122	7	9+10	11.58-12.03	A-7-6(14)	46	22	9.1	47.5	23.3	20.1	98	91	68	
SS-123	7	9+10	13.10-13.55	A-5(0)	43	NP	6.8	52.2	34.9	6.0	100	98	54	
SS-162	-7	9+62	1.09-1.54	A-2-4(0)	19	NP	47.6	44.7	5.7	2.0	100	80	12	
SS-163	-7	9+62	4.13-4.58	A-2-6(0)	31	14	57.8	20.9	5.1	16.1	95	56	22	
SS-164	-7	9+62	7.17-7.62	A-6(5)	39	16	0.5	59.8	13.6	26.2	100	100	51	
SS-165	-7	9+62	8.69-9.14	A-7-6(31)	60	39	4.2	40.0	27.6	28.2	99	96	77	
SS-166	-7	9+62	11.73-12.18	A-7-5(24)	87	26	11.5	24.1	42.3	22.1	100	94	70	
S-303	0	10+00	0.60-1.00	A-3(0)	20	NP	51.2	44.7	2.1	2.0	100	78	7	
S-304	0	10+00	3.80-4.20	A-2-4(0)	14	NP	59.0	25.3	4.5	11.1	96	56	17	
S-305	0	10+00	6.20-6.40	A-2-4(0)	31	10	31.5	44.0	6.4	18.2	96	75	27	
S-306	0	10+00	12.80-13.20	A-6(2)	40	16	30.5	39.9	10.5	19.2	93	75	37	